# MINIMED™ 670G SYSTEM | CHANGING THE MINIMED™ MIO™ ADVANCE INFUSION SET

#### **START HERE**



Wash your hands.
Press O. Select **Options**.

Select Reservoir & Tubing.

Select New Reservoir.

Remove the infusion set you have been using by loosening the adhesive and pulling away from body.



Remove the used reservoir from the pump.


to reduce the risk of air bubbles.

Select Rewind.

plan to fill with insulin.

#### FILL RESERVOIR & CONNECT TO THE INFUSION SET TUBING

Follow the next steps to fill reservoir with insulin and connect to the infusion set tubing.

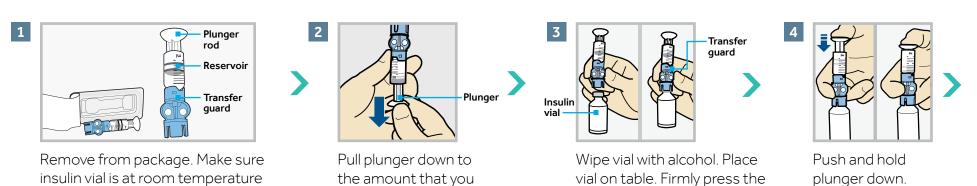

blue transfer guard onto vial.

## MINIMED™ 670G SYSTEM CHANGING THE MINIMED™ MIO™ ADVANCE INFUSION SET

**WARNING** If insulin or any liquid gets inside the tubing connector, it can temporarily block the vents that allow the pump to properly fill the infusion set. This may result in the delivery of too little or too much insulin, which could cause hyperglycemia or hypoglycemia.



With your thumb still on the plunger, flip over so vial is on top. Release thumb and pull plunger down to fill with insulin.



Tap the reservoir to move air bubbles to top of reservoir. Push plunger up to move air into vial.



If needed, pull plunger back down to amount of insulin needed for 2-3 days.



To avoid getting insulin on the top of the reservoir, turn vial over so it is upright. Hold transfer guard and turn reservoir counterclockwise and remove from transfer guard.


#### **CONNECT RESERVOIR TO INFUSION SET**

You will place the tubing connector onto the end of the infusion set to the filled reservoir.







Remove infusion set from package. Remove the paper that holds the tubing together and unwind.



Gently push the tubing connector onto reservoir.
Turn clockwise until locked.
You will hear a click.



If you see air bubbles, tap reservoir to move them to top. Push plunger just a bit to move them into tubing.



Twist plunger counterclockwise to loosen and remove.

# THE BACKLIGHT MAY HAVE TURNED OFF


Press any button to turn the screen back on.



Press O to open the menu. If the pump is locked, you will need to unlock the pump after pressing O.



Select **Load Reservoir** from the menu.




Select Next

Continued on next page

# MINIMED™ 670G SYSTEM | CHANGING THE MINIMED™ MIO™ ADVANCE INFUSION SET

#### PLACE RESERVOIR INTO PUMP

Now place the filled reservoir into the reservoir compartment of the pump.







Place reservoir into pump.



Turn clockwise until you feel reservoir lock into place.



Select Next.

#### LOAD RESERVOIR AND FILL TUBING

Follow these steps to load the reservoir and fill the tubing.




Select **Load** and keep holding O.



When you see this screen, select Next.




Select **Fill** and keep holding O until you see drops at the end of tubing, then let go.



After you see drops, press > and select **Next**.


#### **INSERT INFUSION SET**

Next, follow the steps to insert the infusion set into your body.






Remove the paper backing from the adhesive. Be careful not to touch the adhesive.




Remove the disconnect cover from the insertion device by gently squeezing the sides of the disconnect cover then pulling it away from the insertion device. Keep the disconnect cover for later use.

## MINIMED™ 670G SYSTEM CHANGING THE MINIMED™ MIO™ ADVANCE INFUSION SET

3



Choose an insertion site from the shaded areas shown here. Wipe with alcohol or other antiseptic.



Stretch the skin until smooth. Place the insertion device in the desired location on your skin. The raised arrows indicate the direction to connect the tubing. Press the top button completely down to insert the infusion set.

5




Gently and carefully remove the insertion device by pulling straight away from your body.

6



Press the adhesive onto the skin with your finger. Replace the infusion set if the adhesive does not stick to the skin




Gently hold the cannula housing steady with your finger. Then push the site connector straight into the cannula housing until you hear a click.

Dispose of the insertion device in an appropriate sharps container and in accordance with your local laws.


#### **FILL CANNULA**

You will now fill the cannula, the little tube under your skin, with insulin.



Select Fill.





Select **Fill amount** and enter 0.600 for both the 6mm cannula and 9mm cannula. Then press O.



NOTE: Your pump will remember the Fill amount that you used last. Always verify that the Fill amount is correct.

- If it is correct, press ∨ to **Fill Now** and press ○.
- If it is incorrect, press •. Change to correct amount and press O. Select Fill Now.

# MINIMED™ 670G SYSTEM | CHANGING THE MINIMED™ MIO™ ADVANCE INFUSION SET

Fill Cannula

1. Verify Fill amount.

2. Select Fill Now when ready. Select Back to cancel.

Fill amount 0.600 U

Select Fill Now.

Fill Cannula 0.025

Total: 0.600


The Home screen displays the insulin as it fills the cannula.



**NOTE:** Select **Stop Filling** if you need to stop, for example, if you notice the **Total** amount is incorrect. This should rarely happen if you have verified the **Fill amount** on the previous screen.

Your infusion set change is now complete!

DISCONNECTING THE INFUSION SET FROM YOUR BODY




To disconnect, gently hold the cannula housing steady with your finger. Then squeeze the sides of the site connector and pull it out from the cannula housing.



Put the white cap on the site connector.




3



Put the disconnect cover on the cannula housing. Then push the cover into the cannula housing until you hear a click.

RECONNECTING THE INFUSION SET TO YOUR BODY




Remove the white cap from the site connector by squeezing the side of the site connector then pulling the white cap off.



Ensure there is no air in the tubing. ONLY if there is air in the tubing: Fill the tubing with insulin and watch for drops as instructed. Do not leave any air in the tubing.





Use your finger to gently hold the cannula housing steady. Push the site connector into the cannula housing until you hear a click.